

## Welch Allyn Home™ Blood Pressure Monitor 1500 Series

---



---

### Directions for use

901042 Automated Blood Pressure System  
RPM-BP100

Software version 1.X



© 2017 Welch Allyn. All rights are reserved. To support the intended use of the product described in this publication, the purchaser of the product is permitted to copy this publication, for internal distribution only, from the media provided by Welch Allyn. No other use, reproduction, or distribution of this publication, or any part of it, is permitted without written permission from Welch Allyn. Welch Allyn assumes no responsibility for any injury to anyone, or for any illegal or improper use of the product, that may result from failure to use this product in accordance with the instructions, cautions, warnings, or statement of intended use published in this manual.

The Bluetooth® word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. and any use of such marks by Welch Allyn is under license.

Software in this product is © 2017 Welch Allyn or its vendors. All rights are reserved. The software is protected by United States of America copyright laws and international treaty provisions applicable worldwide. Under such laws, the licensee is entitled to use the copy of the software incorporated with this instrument as intended in the operation of the product in which it is embedded. The software may not be copied, decompiled, reverse engineered, disassembled, or otherwise reduced to human-perceivable form. This is not a sale of the software or any copy of the software; all right, title, and ownership of the software remain with Welch Allyn or its vendors.

For information about any Welch Allyn product, contact Welch Allyn Technical Support: <http://www.welchallyn.com/>

# 726882  
DIR 80022180 Ver. A  
Revised: 2017-04

REF This manual applies to the  
901042 Automated Blood  
Pressure System

Manufactured for Welch Allyn, Inc.  
4341 State Street Road  
Skaneateles Falls, NY 13153 USA

[www.welchallynhome.com](http://www.welchallynhome.com)



## Contents

Contents . . . . .	iii
Introduction . . . . .	1
Indications for use. . . . .	1
Contraindications . . . . .	2
Symbols. . . . .	3
Documentation symbols . . . . .	3
Power symbols . . . . .	3
Shipping, storing, and environment symbols . . . . .	4
Blood pressure device and cuff symbols. . . . .	5
Miscellaneous symbols. . . . .	6
About warnings and cautions. . . . .	8
Warnings and cautions . . . . .	9
Contents list. . . . .	14
Controls and indicators . . . . .	15
Power options . . . . .	17
Screen elements . . . . .	18
Measuring blood pressure. . . . .	21
Overview . . . . .	21
Set up your equipment . . . . .	22
Connect the blood pressure air tube . . . . .	23
Pair a smartphone, a tablet, or a communication hub with the monitor . . . . .	25
Position the blood pressure cuff. . . . .	26
Start the measurement . . . . .	28
Some points to remember about your blood pressure device: . . . . .	31
Disconnect the blood pressure air tube. . . . .	32

Blood pressure facts, pointers, and best practices . . . . .	33
Helpful definitions . . . . .	33
Irregular heartbeat detector . . . . .	33
Maintenance . . . . .	37
Maintain the monitor and cuff . . . . .	37
Troubleshooting . . . . .	38
Problems and error messages . . . . .	38
Technical alarms . . . . .	38
Physiological alarms . . . . .	42
Specifications . . . . .	43
General radio compliance . . . . .	45
Federal Communication Commission (FCC) Interference Statement . . . . .	45
FCC Radiation Exposure Statement . . . . .	47
Industry Canada (IC) compliance . . . . .	47
Complied standards list . . . . .	50
Warranty . . . . .	53
Approved accessories . . . . .	55
Emissions and immunity information . . . . .	57

## **Introduction**

The Welch Allyn Home™ Blood Pressure Monitor 1500 Series (blood pressure monitor) is indicated for adult use in the home or domestic setting only.

The design provides you with two years of reliable service. Readings taken by the monitor are equivalent to those obtained by a trained observer using the cuff and stethoscope auscultation method.

This *Directions for use* contains important safety and care information and provides step by step instructions for using the monitor. Read the manual thoroughly before using the monitor.

## **Indications for use**

The blood pressure monitor is a digital monitor intended for use in measuring blood pressure and heart rate in adult patient populations with arm circumferences between 22 cm to 42 cm (approximately 9 to 17 inches).

The device detects the appearance of irregular heartbeats during measurement and gives a warning signal with readings.

### **Contraindications**

This device is contraindicated for any person who is connected to a wearable or implantable electronic device or instrument, such as a pacemaker or defibrillator.

This blood pressure monitor is not intended to be a diagnostic device. Contact your physician if hypertensive values are indicated.

## Symbols

### Documentation symbols



**Warning:** The warning statements in this manual identify conditions or practices that could lead to illness, injury, or death.



**Caution:** The caution statements in this manual identify conditions or practices that could result in damage to the equipment or other property, or loss of data.



Follow instructions/directions for use (DFU) -- mandatory action

---

### Power symbols



Direct current



Power

---

### Shipping, storing, and environment symbols



Relative humidity limits



Recycle the product separate from other disposables



Temperature limits



Atmospheric air pressure









Recycle











Stacking limit by number

**Blood pressure device and cuff symbols**

 ARTERY	Artery marker
	Range
INDEX 	Index edge
	Limb circumference (Minimum/Maximum)
	Lot code
	Not made with natural rubber latex

### Miscellaneous symbols

---

	Type BF applied part
	Serial number
	Product Identifier
	Manufacturer
	Reorder number, Model number
	Non-ionizing electromagnetic radiation
	Global Trade Identification Number
	Class II equipment

---

---

IP22      Ingress protection: the device is protected against solid foreign objects of 12.5mm and greater and against vertically falling water drops when ENCLOSURE is tilted up to 15°

---



® Bluetooth

---

## About warnings and cautions

Caution statements can appear on the Welch Allyn Home blood pressure device, the packaging, the shipping container, or in this *Directions for use*.

The Welch Allyn Home blood pressure device is safe for adults when used in accordance with the instructions and caution statements presented in this *Directions for use*.

Before using the device, you must familiarize yourself with all cautions, with the steps to power up the device, and with the sections of this *Directions for use* that pertain to your use of the device. In addition to reviewing the general cautions presented in the next section, you must also review the more specific cautions that appear throughout the manual in conjunction with setup/startup, operation, and maintenance tasks.

- Failure to understand and observe any warning statement in this manual could lead to injury or illness.
- Failure to understand and observe any caution statement in this manual could lead to damage to the

equipment or other property, or loss of measurement data.

### Warnings and cautions



**WARNING** Injury risk. The device is not suitable for measuring the blood pressure of neonatal infants or children.

**WARNING** Injury risk. The device is not suitable for use on pregnant women, users with implanted electrical devices, users with preeclampsia, premature ventricular beats, atrial fibrillation, peripheral arterial disease, and users undergoing intravascular therapy or arterio-venous shunt or people who received a mastectomy. Consult your doctor prior to using the unit if you suffer from any of these illnesses or conditions.

**WARNING** Injury risk. Do not take any therapeutic measures on the basis of a self measurement. Never alter the dose of a medicine prescribed by a doctor. Consult your doctor if you have any question about your blood pressure.

**WARNING** Injury risk. Keep the unit out of reach of infants, children, or pets, since inhalation or swallowing of small parts is dangerous or even fatal.



**WARNING** Injury risk. The device is not intended to be a self-measurement station used in a public place or center.

**WARNING** Injury risk. Do not burn batteries. Batteries may leak or explode.

**WARNING** Injury risk. If you experience discomfort during a measurement, such as pain in the arm or other complaints, press the power button immediately to release the air from the cuff. Loosen and remove the cuff from your arm.

**WARNING** Injury risk. On the rare occasion of a fault causing the cuff to remain fully inflated during measurement, open the cuff immediately. Prolonged high pressure applied to the arm (cuff pressure >300mmHg or constant pressure >15mmHg for more than 3 minutes) might lead to bruising and discolored skin.

**WARNING** Injury risk. This unit is not suitable for continuous monitoring during medical emergencies or operations.

**WARNING** Injury risk. Taking blood pressure measurements too frequently could disrupt blood circulation and cause injuries.



WARNING Injury risk. Do not kink the connection tube during use. The cuff pressure might continuously increase, which could prevent blood flow and result in injury.

WARNING Injury risk. Never apply the cuff over damaged skin. This can cause further injury.

WARNING Injury risk. If applying to someone else, do not touch output of the batteries/adaptor and the user simultaneously.

WARNING Injury risk. Do not use the unit if you are allergic to polyester or synthetic materials.

WARNING Injury risk. Excessive tube lengths could cause strangulation if you don't manage them properly.

WARNING Injury risk. Do not connect the air tube to other medical equipment. This could cause air to be pumped into intravascular systems or high pressure, which could lead to serious injuries.

WARNING Injury risk. Dispose of accessories, detachable parts, and the device according to the local guidelines.



WARNING Injury risk. Do not service or perform any maintenance while using the device.

WARNING Injury risk. Use only accessories approved by the manufacturer. Using unapproved accessories might cause damage to the unit and injure users.

WARNING Injury risk. No modification to this equipment is allowed. Modifying the equipment could damage the unit or endanger the user.



Caution This device is intended for non-invasive measuring and monitoring of arterial blood pressure. It is not intended for use on extremities other than arm or for functions other than obtaining a blood pressure measurement.

Caution Do not wrap the cuff on the same arm to which another monitoring device is applied. One or both devices could temporarily stop functioning if you try to use them on the same arm at the same time.

Caution To avoid measurement errors, avoid taking blood pressure measurements near a strong electromagnetic field radiated interference signal or electrical fast transient/burst signal.

Caution The materials of the cuff have been tested and found to comply with requirements of ISO 10993-5:2009 and ISO 10993-10:2010. It will not cause any potential sensitization or irritation reaction.

Caution Before use, make sure the device functions safely and is in proper working condition.

Caution Use the device in the environment described in this directions for use. Otherwise, you will compromise the device's performance and reduce its lifetime.



Caution Do not attempt to repair the unit yourself if it malfunctions. Only have repairs carried out by authorized service centers.

Caution Report any unexpected operation or events to the manufacturer.

Caution Use a soft cloth to clean the entire unit. Do not use any abrasive or volatile cleaners. See the cleaning instructions presented later in this *Directions for use*.


### Contents list

The following items are in the device box:

- Blood Pressure Monitor
- D-Ring Standard Wide Cuff (22cm to 42cm / 9in to 17in) with air tube attached
- (4) AA alkaline batteries
- Directions for use
- Quick reference guide

## Controls and indicators


### Monitor front

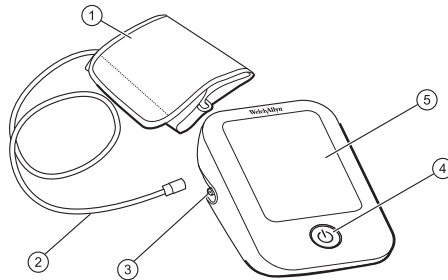

No.	Feature	Description
1	D-Ring blood pressure cuff	Apply to upper arm to take a blood pressure measurement
2	Air tube	Connects the cuff to the air connector plug
3	Air connector plug	Air tube connects to the air connector plug
4	Power button	Powers on the monitor, starts and stops a blood pressure measurement, and — when pressed for 2 seconds — initiates a <i>Bluetooth</i> pairing

No.	Feature	Description
5	LCD Display	Displays blood pressure reading and other pertinent information regarding the reading

**Monitor back**

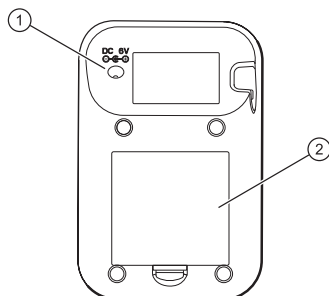


No.	Feature	Description
1	Direct current power connection	When used with an accessory power cord (not included), connects the monitor to a power outlet
2	Battery compartment (behind cover)	Houses 4 AA alkaline batteries

## Power options



Caution To get optimal performance and protect your monitor, use only the correct batteries or the Welch Allyn-approved power adapter.








The monitor is powered by one of two sources:





- 4 AA alkaline batteries
- AC adapter (6v  1A) (not included)

### Screen elements

The liquid crystal display (LCD) displays the following: systolic blood pressure (mmHg), diastolic blood pressure (mmHg), pulse rate (bpm), heart beat (regular or irregular) while acquiring blood pressure measurements, excessive motion alert, *Bluetooth* connectivity status or data transmission error, alarm priority, and battery charge level.



Symbol	Description
	Systolic blood pressure mmHg = measurement unit of the blood pressure
	Diastolic blood pressure mmHg = measurement unit of the blood pressure
	Pulse in beats per minute
	Irregular heartbeat Monitor is detecting an irregular heartbeat during measurement
	Heart beat Monitor is detecting a heartbeat during measurement
	Battery indicator Indicates the current battery charge
	Battery indicator Indicates the current battery charge

Symbol	Description
	<i>Bluetooth</i> connectivity status or data transmission error
	Motion indicator Motion may result in an inaccurate measurement.
	Reading out of range Either SYS > 260mmHg or DIA > 220mmHg. The symbol may appear in either the SYS or DIA area of the screen. Alarm priority = Low (an! appears near the top of the screen)
	Reading out of range Either SYS < 50mmHg or DIA < 25mmHg. The symbol may appear in either the SYS or DIA area of the screen. Alarm priority = Low (an! appears near the top of the screen)

## Measuring blood pressure

### Overview

You are the intended operator of the device. You can measure your blood pressure and then save and send measurement data to a smartphone or tablet. You can also maintain your device and its accessories, and you can change the batteries under normal circumstances.

To measure your blood pressure, you need the following:

- Blood pressure monitor with batteries inserted
- Blood pressure cuff ("D-ring" style for easy, one-handed adjustment)
- Blood pressure air tube

To save and transfer blood pressure measurements, you also need a smartphone or tablet with *Bluetooth* wireless connectivity and the application or software to receive your data, such as the Welch Allyn Home application or another healthcare provider application.

## Set up your equipment

### Insert or replace the batteries



**WARNING** Injury risk. Do not burn batteries. Batteries may leak or explode.



**Caution** Remove the batteries if the device is not used regularly.  
**Caution** Dispose of old batteries by following your local recycling guidelines.


If you are not using AC power, you must install 4 AA alkaline batteries before using the device.

Replace the batteries when any of the following occurs:

- The battery charge indicator indicates a low charge
- The display dims
- The display does not light up

1. Slide off the battery cover.

2. Install the batteries by matching the polarity as shown in the diagram.

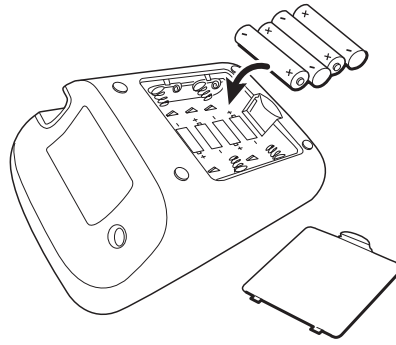


3. Replace the cover.

### **Connect the blood pressure air tube**

1. Locate the air connector plug on the left side of the blood pressure monitor.

2. Place your thumb and forefinger on the metal air tube connector and slide it onto the air connector plug.

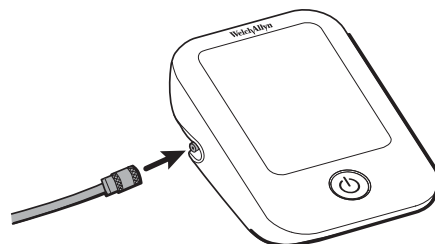

3. Confirm that the air tube connector locks into place. Listen for a click.

When the air tube connector is properly seated, you cannot pull it off the air connector plug.

**Note** You may leave the air tube connected to the blood pressure monitor if you take your blood pressure regularly and have a convenient place to store the blood pressure monitor and cuff together without kinking the tube.

### **Pair a smartphone, a tablet, or a communication hub with the monitor**



Advanced *Bluetooth* 4.0 technology enables your smartphone, your tablet, or a communication hub to receive your personal health information from your blood pressure monitor. You have two alternatives to pair the monitor with these devices:

- If you are using the Welch Allyn Home application, follow the pairing instructions presented in the application.
- Contact your Remote Monitoring Solution provider or use the instructions that office provided to set up these communications devices.

With either alternative, you complete the same steps on the monitor:

1. Confirm that smartphone, tablet, or communication hub is powered on and in discoverable mode (ready for pairing). *Bluetooth* wireless connectivity is only available for devices which support *Bluetooth* 4.0 technology.
2. Press and hold the Power button on the blood pressure monitor for 2

seconds to power on the device and activate *Bluetooth* pairing. The *Bluetooth* symbol flashes while discovering the monitor.

If successful, a steady  symbol surrounded by a dotted line appears on the LCD screen. If unsuccessful, the  appears.


### **Position the blood pressure cuff**

To achieve an accurate blood pressure reading, follow these steps to position the blood pressure cuff properly.


1. Remove any sleeves covering your upper arm.

**Note** The preferred site for taking a blood pressure measurement is your bare upper arm.


2. Place the cuff loosely over your arm so that the blood pressure tube extends down over your hand. It should appear on your arm as shown.

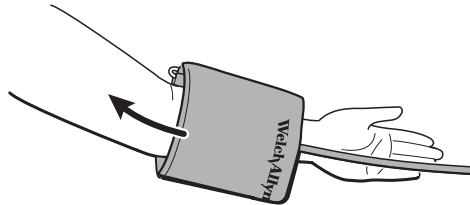

3. Open the cuff to resize it as needed and slide it over your bare upper arm. The bottom edge of the cuff should be 2 to 3 centimeters (0.8 to 1.2 inches) above the bend in your arm, and the tube and artery marker should appear on your arm as shown.

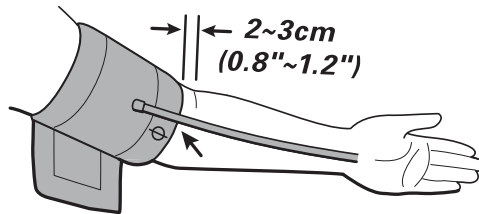

4. Keeping the artery marker and the tube in place, wrap the cuff snugly around your arm, but not too tight. If you can insert just two fingers between the cuff and your arm, the tightness is acceptable.

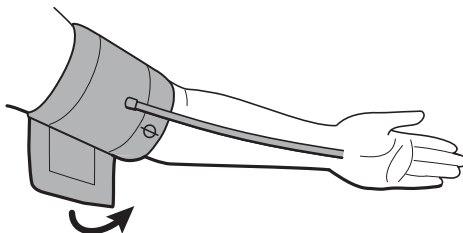

**Start the measurement**

1. Prepare yourself to take your blood pressure.
  - a. Sit comfortably in a chair that supports your back.
  - b. Keep legs uncrossed.
  - c. Place feet flat on the floor.
  - d. Support your arm on the flat surface.

- e. Ensure the cuff is level with your heart (right atrium).
  - f. Rest for 5 minutes after sitting down and positioning the blood pressure cuff.
2. Verify that the cuff is positioned correctly with the tube running down the middle of your forearm.
  3. Press the **Power** button to power up the monitor and begin the blood pressure measurement.

The cuff inflates and tightens around your arm until it completes the measurement. A vertical stack of segments appears onscreen to show increasing pressure in the cuff. The heart icon in the upper-left corner blinks to indicate your pulse rate until the measurement is complete.

Note If you press the Power button to stop the measurement, dotted lines replace the SYS and DIA numbers onscreen.

When the inflation cycle is complete, systolic and diastolic measurements as well as your pulse rate appear onscreen.

4. Record your measurement results. Either record these measurements manually along with the time of measurement, or transfer them electronically to your connected device.



Caution The device that receives transferred measurements displays the most recent record first as record 1. Each new measurement becomes record 1, and all other records move down the list (for example, 2 becomes 3, and so on). You can store a maximum of 99 records. When you pass that limit, the oldest record drops from the list.

Note For a meaningful comparison, try to take measurements under consistent conditions. For example, take daily measurements at approximately the same time, on the same upper arm, or as directed by your physician.


**Some points to remember about your blood pressure device:**

- After 10 seconds of inactivity, the device powers down.
- If you press and release the Power button, the device powers down.
- After successful transfer, the device powers off the *Bluetooth* radio, and the *Bluetooth* icon (and rectangle) disappear.

### Disconnect the blood pressure air tube

**Note** You may leave the air tube connected to the blood pressure monitor if you take your blood pressure regularly. Store the monitor and cuff in a convenient place; do not kink the tube.

1. If you choose to disconnect the air tube after completing a blood pressure measurement, place your thumb and forefinger on the grooved portion of the metal air tube connector and pull it back. Do not twist the connector.

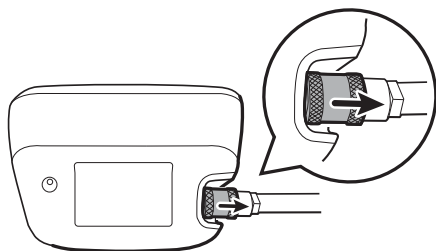

2. Gently pull the air tube away from the monitor. You can now store the monitor and the cuff.

## **Blood pressure facts, pointers, and best practices**

### **Helpful definitions**

**Systolic pressure** When ventricles contract and pump blood out of your heart, the point at which blood pressure reaches its maximum value in the cycle.

**Diastolic pressure** When the ventricles relax, the point at which blood pressure reaches its minimum value in the cycle.

**Pulse rate** A measurement of the heart rate, or the number of times the heart beats per minute. As the heart pushes blood through the arteries, the arteries expand and contract with the flow of the blood.

### **Irregular heartbeat detector**

An irregular heartbeat (IHB) is detected when a heartbeat rhythm varies while the unit is measuring the systolic and diastolic blood pressure. During each measurement, the monitor records the heartbeat intervals and calculates the average. If any average is larger than or equal to 25%, the irregular heartbeat symbol appears on the display when the measurement results appear.



Caution The appearance of the IHB icon indicates that a pulse irregularity consistent with an irregular heartbeat was detected during measurement. Usually this is NOT a cause for concern. However, if the symbol appears often, we recommend you seek medical advice. The device does not replace a cardiac examination but detects pulse irregularities at an early stage.

### Why does my blood pressure fluctuate throughout the day?

- Individual blood pressure varies multiple times every day because of weather, emotion, and activity.
- The way you position your cuff and your measurement posture can affect blood pressure. Try to take blood pressure measurements under similar conditions.
- Sometimes blood pressure on one arm is different from blood pressure on your other arm. Use the same arm for blood pressure measurements.
- Medication might affect your blood pressure.
- The "white coat effect" might cause your blood pressure to be higher in a hospital or doctor's office.

### Factors that could cause inaccurate measurements

- Cuff position is poor
- Cuff is too loose or too tight
- Cuff is applied over clothing rather than on a bare upper arm
- Taking a measurement within 1 hour of eating or drinking
- Taking a measurement within 20 minutes of taking a bath
- Being in a cold environment
- Taking a measurement immediately after smoking or drinking caffeinated beverages
- Taking a measurement while talking or moving your fingers
- Taking a measurement when you need to urinate
- Taking measurements in rapid succession

### Factors that promote accurate blood pressure measurements

- Proper cuff position on the upper arm
- Proper cuff tightness
- No clothing under the cuff or restricting circulation above the cuff
- Proper posture: feet flat on the floor, back straight, legs uncrossed, arm resting on a flat surface, upper arm at heart level
- Relaxing or sitting still for a few minutes after positioning the cuff

and before taking a blood pressure measurement

- Sitting still during measurement
- Not talking during measurement
- Waiting at least 3 minutes between measurements

## Maintenance

### Maintain the monitor and cuff

The monitor does not require calibration.

To get the best performance from your monitor, follow the maintenance steps below.

- Store the unit in a dry place away from direct sunlight.
- Avoid shaking and dropping the monitor.
- Avoid operating the monitor in dusty and unstable temperature environments.

### Cleaning



Caution Use a soft cloth to clean the entire unit. Do not use any abrasive or volatile cleaners.

1. Clean the monitor only when necessary with one of the following compatible cleaning agents:
  - 70% isopropyl alcohol
  - 10% chlorine bleach/90% water solution (standard bleach wipe)
2. If necessary, you may wipe the cuff with a soft, damp cloth.

## Troubleshooting

This section includes a list of error messages and frequently asked questions for problems you may encounter with your blood pressure monitor. If the device is not operating as you think it should, check here before arranging for service.

### Problems and error messages

The device presents technical alarms and low-priority physiological alarms. Technical alarms occur when there is a device-related error. Physiological alarms occur when blood pressure measurements fall outside of set alarm limits.

### Technical alarms

<b>Problem</b>	<b>Symptom</b>	<b>Root cause</b>	<b>Solution</b>
No power	Display will not light up	Batteries are drained.	Replace with new batteries
		Batteries are inserted incorrectly.	Insert the batteries correctly
		AC adapter is inserted incorrectly	Insert the AC adapter tightly

<b>Problem</b>	<b>Symptom</b>	<b>Root cause</b>	<b>Solution</b>
Low batteries	The display indicates the "BAT-LO" message, pauses for 3 seconds. The battery icon shows empty (does not flash.)	Batteries are low.	Replace with new batteries
Error messages	E 01 shows	The cuff is not secure	Readjust the cuff, relax for a moment, and then measure again
	E 02 shows	The cuff is very tight	Refasten the cuff and then measure again
	E 03 shows	There is too much pressure in the cuff	Refasten the cuff and then measure again
	E 10 or E 11 shows	The monitor detected motion while measuring	Readjust the cuff, relax for a moment, and then measure again



<b>Problem</b>	<b>Symptom</b>	<b>Root cause</b>	<b>Solution</b>
	E 20 shows	The measurement process does not detect a pulse signal	Loosen the clothing on the arm and then measure again
	E 21 shows	The measurement is incorrect	Relax for a moment and then measure again
	EE or E 19 shows	Hardware error	Measure again. If the problem persists, contact the retailer or Welch Allyn customer service at <a href="http://www.welchallynhome.com">www.welchallynhome.com</a> for further assistance.

---

<b>Problem</b>	<b>Symptom</b>	<b>Root cause</b>	<b>Solution</b>
----------------	----------------	-----------------------	-----------------

Visit [www.welchallynhome.com](http://www.welchallynhome.com) for further assistance.

## Physiological alarms

Symptom	Root cause	Solution
	Out of range. Either SYS >260mmHg or DIA >220mmHg. The symbol may appear in either the SYS or DIA area of the screen.	Press and hold the <b>Power</b> button to reestablish <i>Bluetooth</i> connectivity. Measure again. If the problem persists, contact your physician.  Alarm priority = Low
	Out of range. Either SYS <50mmHg or DIA <25mmHg. The symbol may appear in either the SYS or DIA area of the screen.	Press and hold the <b>Power</b> button to reestablish <i>Bluetooth</i> connectivity. Measure again. If the problem persists, contact your physician.  Alarm priority = Low

## Specifications

Item	Specification
Power supply: Battery powered mode:	6VDC 4*AA batteries
Power supply: AC adapter powered mode:	Input: 100-240V, 50- 60Hz, 400mA; Output: 6V, 1A
Power supply model number	UE08WCP-06100SPA
Display mode	Digital LCD V.A.68mm*90mm
Measurement model	Oscillometric testing mode
Measurement range	Rated cuff pressure: 0mmHg to 300mmHg (0kPa- 40kPa) Measurement pressure: SYS: 60 to 230mmHg DIA: 40 to 130mmHg Pulse value: (40 to 199)beat/minute
Accuracy	Pressure: ±0.4kPa (3mmHg) Pulse value:±4%

44 Welch Allyn Home Blood Pressure Monitor

<b>Item</b>	<b>Specification</b>				
Normal working conditions	Temperature: 5°C to 40°C Relative humidity 85% RH Atmospheric pressure: 86kPa to 106kPa				
Storage and transportation condition	Temperature:-20°C to 60°C Relative Humidity: 10% RH-93% RH Atmospheric Pressure: 50kPa to 106 kPa				
Circumference of the upper arm	<table border="1"> <thead> <tr> <th>Part Number</th> <th>Cuff size</th> </tr> </thead> <tbody> <tr> <td>Standard wide = RPM-BPACC-02</td> <td>22cm to 42cm Approximately 9in to 17in</td> </tr> </tbody> </table>	Part Number	Cuff size	Standard wide = RPM-BPACC-02	22cm to 42cm Approximately 9in to 17in
Part Number	Cuff size				
Standard wide = RPM-BPACC-02	22cm to 42cm Approximately 9in to 17in				
Net Weight	Approx. 283g (Excluding the dry cells)				
External dimensions	Approx. 94mm *142mm*66mm				
Degree of protection	Type BF applied part				
Protection against ingress of water	IP22				
Software Version	Version 1.X				

## General radio compliance

Item	Specification
<i>Bluetooth</i> Module No.	AW2540MV1
Radio Frequency (RF) Range	2402 MHz to 2480 MHz
Output Power	-1.0 dBm
Supply Voltage	2.0 to 3.6V
Antenna Gain	0.0 dBi
Transmitting Distance	10 meters (30 feet)

## Federal Communication Commission (FCC) Interference Statement

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions.

- This device may not cause harmful interference.
- This device must accept any interference received, including interference that may cause undesired operation.

This equipment (FCC ID: OU9TMB1591-B) has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC

Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one of the following measures.

1. Reorient or relocate the receiving antenna.
2. Increase the separation between the equipment and receiver.
3. Consult the dealer or an experienced radio/TV technician for help.

Any changes or modifications not expressly approved by the party responsible for compliance could

void the user's authority to operate this equipment.

### **FCC Radiation Exposure Statement**

This equipment complies with FCC radiation exposure limits set forth for an uncontrolled environment. This transmitter must not be co-located or operating in conjunction with any other antenna or transmitter.

### **Industry Canada (IC) compliance**

To ensure compliance with FCC and Industry Canada RF exposure requirements, this device must be installed in a location where the antennas of the device will have a minimum distance of at least 20 cm from all persons. Using higher gain antennas and types of antennas not certified for use with this product is not allowed. The device shall not be co-located with another transmitter.

Pour s'assurer de la conformité des exigences aux expositions RF de la FCC et de l'Industry Canada, cet appareil doit être installé dans un emplacement où les antennes de l'appareil sont au moins à 20 cm de distance de toute personne. L'utilisation d'antennes et de types

d'antennes à gain supérieur non garantis avec ce produit est interdite. L'appareil ne doit pas être installé à proximité d'un autre émetteur.

This device complies with Industry Canada licence-exempt RSS standard(s). Operation is subject to the following two conditions: (1) this device may not cause interference, and (2) this device must accept any interference, including interference that may cause undesired operation of the device.

Cet appareil est conforme aux normes RSS exemptes de licence de l'Industry Canada. Son fonctionnement est soumis aux deux conditions suivantes: (1) l'appareil ne doit pas produire de brouillage, et (2) l'appareil doit accepter tout brouillage radioélectrique subi, même si le brouillage est susceptible d'en compromettre le fonctionnement.

This radio transmitter (IC: 12725A-TMB1591B) has been approved by Industry Canada to operate with the antenna listed in the specification table.

Ce transmetteur de radio (IC: 12725A-TMB1591B) a été approuvé par l'Industry Canada pour fonctionner avec l'antenne

répertoriée dans la table des spécifications.

This Class B digital apparatus complies with Canadian ICES-003.

Cet appareil numérique de la classe B est conforme à la norme NMB-003 du Canada.

**Complied standards list**

<b>Item</b>	<b>Standard</b>
Risk management	ISO/EN 14971 Medical devices — Application of risk management to medical devices
Labeling	ISO/EN 15223-1 Medical devices. Symbols to be used with medical device labels, labeling and information to be supplied. General requirements
User manual	EN 1041 Medical equipment manufacturers to provide information
General Requirements for Safety	IEC 60601-1+A1 Medical electrical equipment - Part 1: General requirements for basic safety and essential performance  IEC 60601-1-11 Medical electrical equipment - Part 1-11: General requirements for basic safety and essential performance - Collateral standard: Requirements for medical electrical equipment and medical electrical systems used in the home healthcare environment

<b>Item</b>	<b>Standard</b>
Electromagnetic compatibility	IEC/EN 60601-1-2 Medical electrical equipment - Part 1-2: General requirements for basic safety and essential performance - Collateral standard: Electromagnetic compatibility - Requirements and tests
Performance requirements and clinical investigation	IEC 80601-2-30 Medical electrical equipment- Part 2-30: Particular requirements for the basic safety and essential performance of automated non-invasive sphygmomanometers  ISO81060-2:2013 Non-invasive sphygmomanometers — Part 2: Clinical validation of automated measurement type
Software life-cycle processes	IEC/EN 62304+AC: Medical device software - Software life cycle processes

52 Welch Allyn Home Blood Pressure Monitor

<b>Item</b>	<b>Standard</b>
Usability	IEC 62366 Medical devices - Application of usability engineering to medical devices (IEC 62366)  IEC 60601-1-6 Medical electrical equipment - Part 1-6: General requirements for basic safety and essential performance - collateral standard: Usability

## **Warranty**

Welch Allyn will warranty the blood pressure monitor to be free of defects in material and workmanship and to perform in accordance with manufacturer specifications for the period of two years from the date of purchase from Welch Allyn or its authorized distributors or agents.

The warranty period shall start on the date of purchase. The date of purchase is: 1) the invoiced ship date if the device was purchased directly from Welch Allyn, 2) the date specified during product registration, 3) the date of purchase of the product from a Welch Allyn authorized distributor as documented from a receipt from said distributor.

This warranty does not cover damage caused by: 1) handling during shipping, 2) use or maintenance contrary to labeled instructions, 3) alteration or repair by anyone not authorized by Welch Allyn, and 4) accidents.

The product warranty is also subject to the following terms and limitations.


- Accessories are not covered by the warranty.
- Shipping cost to return a device to a Welch Allyn service center is not included.
- A service notification number must be obtained from Welch Allyn prior to returning any products or accessories to Welch Allyn's designated service centers for repair. To obtain a service notification number, contact Welch Allyn Technical Support at [www.welchallynhome.com/support](http://www.welchallynhome.com/support).

## Approved accessories

<b>Item</b>	<b>Description</b>
RPM-BPACC-02	D-Ring Standard Wide Cuff (22-42cm)
RPM-BPACC-04	RPM BP AC Adapter. This adapter is an alternate power source for the blood pressure monitoring device.



## Emissions and immunity information


Electromagnetic emissions	
<p>The Welch Allyn Home Blood Pressure Monitor BPM-BP100 is intended for use in the electromagnetic environment specified below. The customer or user of the Welch Allyn Home Blood Pressure Monitor should assure that it is used in such an environment.</p>	
<p> <b>Caution</b> Wireless communications equipment, such as wireless home network devices, mobile phones, cordless telephones and their base stations, walkie-talkies can affect this equipment and should be kept at least a distance d=3,5m away from the equipment.</p>	
<p><b>Note</b> As indicated in Table 6 of IEC 60601-1-2:2007 for ME Equipment, a typical cell phone with a maximum output power of 2 W, yields d=3,3m at an IMMUNITY LEVEL of 3V/m).</p>	
Emissions test	Compliance
RF emissions CISPR 11	Electromagnetic environment - guidance Group 1
<p>The Welch Allyn Home Blood Pressure Monitor uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.</p>	

Electromagnetic emissions	
RF emissions	Class B
CISPR 11	The Welch Allyn Home Blood Pressure Monitor is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions	
IEC 61000-3-2	
Voltage fluctuations/flicker emissions	
IEC 61000-3-3	

Electromagnetic immunity			
The Welch Allyn Home Blood Pressure Monitor is intended for use in the electromagnetic environment specified below. The customer or the user of the Welch Allyn Home Blood Pressure Monitor should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±6 kV contact ± 8kV air	±6 kV contact ± 8kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	± 1 kV line(s) to line(s) ± 2kV line(s) to earth	± 1 kV differential mode	Mains power quality should be that of a typical commercial or hospital environment.

Electromagnetic immunity	
<p>Voltage dips, short interruptions and voltage variations on power supply input lines</p> <p>IEC 61000-4-11</p>	<p>&lt; 5% <math>U_T</math></p> <p>(&gt;95% dip in <math>U_T</math>) for 0.5 cycle</p> <p>40% <math>U_T</math></p> <p>(60% dip in <math>U_T</math>) for 5 cycles</p> <p>70% <math>U_T</math></p> <p>(30% dip in <math>U_T</math>) for 25 cycles</p> <p>&lt; 5% <math>U_T</math></p> <p>(&gt;95% dip in <math>U_T</math>) for 5 seconds</p>
<p>Power frequency (50HZ) magnetic field</p> <p>IEC 61000-4-8</p>	<p>3A/m</p> <p>3A/m</p>
<p>Mains power quality should be that of a typical commercial or hospital environment. If the user of the Welch Allyn Home Blood Pressure Monitor requires continued operation during power mains interruptions, it is recommended that the Welch Allyn Home Blood Pressure Monitor be powered from an uninterruptible power supply or a battery.</p> <p>Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.</p>	
<p>Note: <math>U_T</math> is the AC mains voltage prior to application of the test level.</p>	

Electromagnetic immunity		
The Welch Allyn Home Blood Pressure Monitor is intended for use in the electromagnetic environment specified below. The customer or the user of the Welch Allyn Home Blood Pressure Monitor should assure that it is used in such an environment.		
Immunity test	IEC 60601 test level	Compliance level Electromagnetic environment - guidance
Portable and mobile RF communications equipment should be used no closer to any part of the Welch Allyn Home Blood Pressure Monitor, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.		
Recommended separation distance		
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz	3 Vrms
		$d = 1.2 \sqrt{P}$

Electromagnetic immunity	
Radiated RF	3 V/m
IEC 61000-4-3	80 MHz to 1 GHz
	$d = 1.2 \sqrt{P}$ 80 to 800 MHz
	$d = 2.333 \sqrt{P}$ 800 MHz to 2.5 GHz
<p>where <math>P</math> is the maximum output power rating of the transmitter in watts (W) and <math>d</math> is the recommended separation distance in meters (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey<sup>a</sup> should be less than the compliance level in each frequency range<sup>b</sup>. Interference may occur in the vicinity of equipment marked with the following symbol:</p>	
	

---

### Electromagnetic immunity

---

Note 1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

<sup>a</sup>Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless), telephones and land mobile radios, amateur radio, AM and FM radio broadcast, and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Welch Allyn Home Blood Pressure Monitor is used exceeds the applicable RF compliance level above, the Welch Allyn Home Blood Pressure Monitor should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the Welch Allyn Home Blood Pressure Monitor.

<sup>b</sup>Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

---

Recommended separation distances between portable and mobile RF communications equipment and the Welch Allyn Home Blood Pressure Monitor

The Welch Allyn Home Blood Pressure Monitor is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or user of the Welch Allyn Home Blood Pressure Monitor can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the Welch Allyn Home Blood Pressure Monitor as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of transmitter (W)	Separation distance according to frequency of transmitter (m)		
	150 kHz to 80 MHz	80 MHz to 800 MHz	800 MHz to 2.5 GHz
	$d = 1.2 \sqrt{P}$	$d = 1.2 \sqrt{P}$	$d = 2.3 \sqrt{P}$
0.01	0.167	0.167	0.2333
0.1	0.369	0.369	0.738
1	1.167	1.167	2.333
10	3.690	3.690	7.338
100	11.67	11.67	23.33

---

Recommended separation distances between portable and mobile RF communications equipment and the Welch Allyn Home Blood Pressure Monitor

---

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where  $P$  is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

Note 1: At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

Note 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

---





Welch Allyn® Home™  
Blood Pressure Monitor

Model: RPM-BP100

# 726882  
DIR 80022180 Ver. A

